



Solartron  
Metrology

## ABSOLUTE TTL MODULE



user leaflet


**AMETEK**<sup>®</sup>  
ULTRA PRECISION TECHNOLOGIES

# Product Description

---

## Introduction

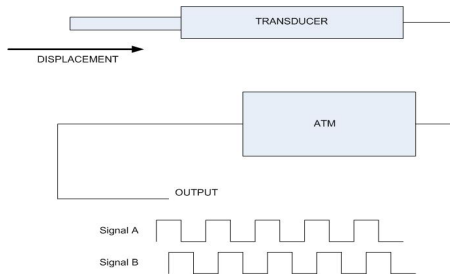

The Solartron ATM transducer comprises a sensor and conditioning electronics which provides an RS422 level square wave output. Each output pulse represents a discrete incremental displacement.



This type of square wave output, often called TTL can be read by many basic counter cards and instruments.

The major difference between the ATM and conventional incremental sensors which provide outputs of this type is that the ATM is an absolute sensor and therefore cannot lose its position even if it is moved quickly. Incremental sensors will miss count if moved too quickly, which means they need a reference signal at a known position to re-date. The ATM does not need this and does not provide a reference signal.

# Safety

<p><b>WARNING</b> statements identify conditions or practices that could result in personal injury or loss of life</p> <p><b>CAUTION</b> statements identify conditions or practices that could result in damage to the equipment or other property</p>		<p><b>Warnings and Cautions</b></p> <p><b>Warning:</b> do not operate in an explosive atmosphere.</p> <p><b>Warning:</b> this equipment is not intended for safety critical applications.</p> <p><b>Warning :</b> do not exceed the maximum ratings as specified in this document</p> <p>This equipment operates below the SELV and is therefore outside the scope of the Low Voltage Directive</p>	
<p><b>Symbols in this manual</b></p>		<p><b>Service and Repair</b></p>	
	Indicates cautionary or other information		No user serviceable parts. Return to supplier for repair

# Operation

---

## Output Signals Provided

The ATM provides four output signals in the form of square waves. These are Signals A and B. Signal B is phase shifted 90 degrees to Signal A. For each signal A and B the inverse signal is also transmitted.

The Signal A and the inverse signal A is often called a Differential Signal A and the Signal B and the inverse signal B a Differential Signal B.

Signal A is commonly referred to as the IN PHASE Signal and Signal B as the QUADRATURE Signal, where quadrature indicates a 90 degree phase shift with respect to the in phase signal.

# Operation

---


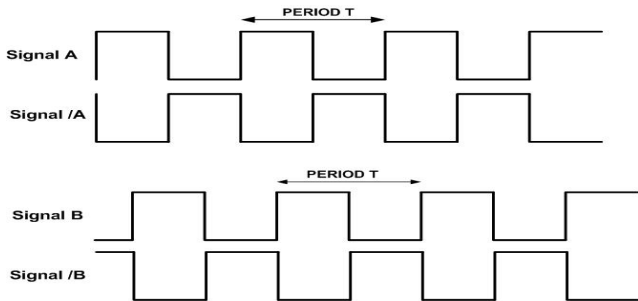


Figure 2: Output Signal Waveforms

The period of Signal A and Signal B is the same and therefore the Output Signal Frequency of A and B is:-

$$\text{Output Signal Frequency} = 1/\text{PERIOD} = 1/T$$

# Resolution

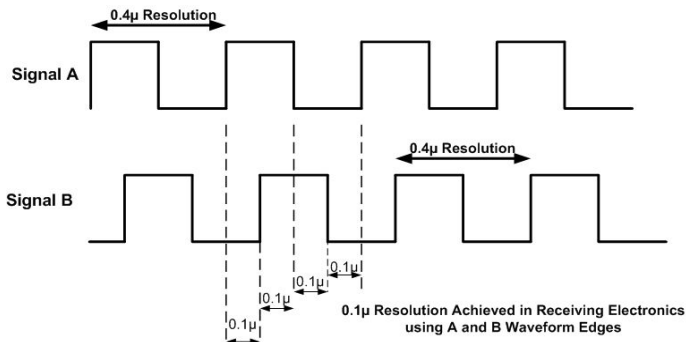

In figure 2 the period  $T$  of the signal corresponds to the resolution of the ATM. The ATM can be factory set to a specified resolution. These are  $0.1 \mu\text{s}$ ,  $0.2 \mu\text{s}$  and  $0.5 \mu\text{s}$ . **The resolution assumes x4 interpolation in the receiving electronics. (see opposite Fig 3).**

The period  $T$  of the separate A and B signals is therefore  $0.4 \mu\text{s}$ ,  $0.8 \mu\text{s}$ ,  $2 \mu\text{s}$ .

# Direction of Count Pulses

---

For an inward displacement Signal A leads Signal B,

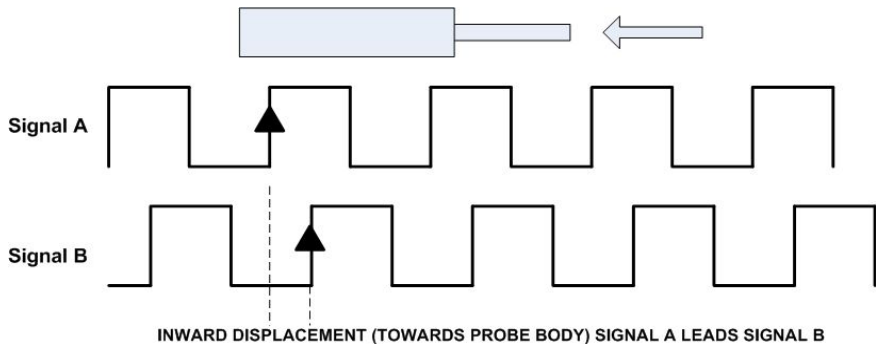


Fig 4a

# Direction of Count Pulses

---

For an outward displacement Signal B leads Signal A

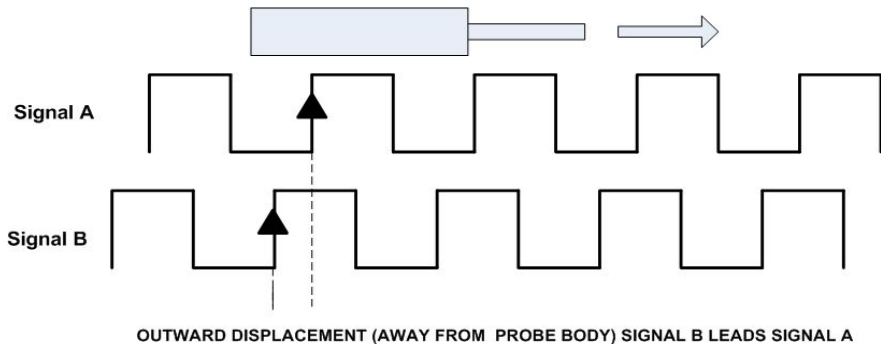


Fig 4b



# Transmission of Count Pulses and Receiver Requirements

---

## Number of Pulses sent

The ATM will send the exact number of pulses corresponding to the displacement moved. This will depend on the resolution set.

Number of A and B Pulses = Displacement ( $\mu\text{m}$ ) / Selected resolution x 4.

E.g. Selected Resolution = 0.1  $\mu\text{m}$ . Displacement = 1.5 mm

Number of A and B Pulses =  $(1.5 \times 1000) / (0.1 \times 4) = 3750$  pulses.

The receiving electronics must be able to count x4 the Number of pulse edges to correctly count the pulses. (See Fig 3).

# Frequency of Pulses

---

Three factors affect the output frequency of Signals A and B from the ATM, these are:

- Maximum Output Signal Frequency, which is factory set. The ATM will never transmit at a higher frequency than this setting.
- The ATM resolution.
- The speed at which the probe is moved.

The output frequency of Signals A and B is calculated from the equation.

$$\text{Output frequency} = \frac{\text{Rate of change of Displacement (mm/sec)} * 1000}{\text{ATM Resolution} \times 4}$$

# Frequency of Pulses

---

Three factors affect the output frequency of Signals A and B from the ATM, these are:

Table 1 below shows the relationship between Rate of change of Displacement (how fast the probe is moving) and the Output frequency for an ATM with a factory set resolution of 0.1  $\mu\text{m}$  and a factory set maximum Output Frequency of 100 kHz.




Rate of Change of displacement	ATM Resolution	Output Frequency	
mm/sec	$\mu\text{m}$	Hz	
1	0.1	2500	
2	0.1	5000	
5	0.1	12500	
10	0.1	25000	
20	0.1	50000	
50	0.1	100000	
100	0.1	100000	

Output Frequency Limited by maximum Output Signal Frequency

Table 1: Rate of Change of Displacement and Output Frequency

# Frequency of Pulses

Example: Output Waveforms. (ATM set to 0.1  $\mu\text{m}$  resolution, Max Output Frequency = 100 kHz)

 <p>400<math>\mu\text{s}</math> (2500Hz)</p> <p>10<math>\mu\text{s}</math> (100kHz)</p>	<p>Probe moving at 1 mm/sec, therefore 2500 A pulses per second.</p>
 <p>200<math>\mu\text{s}</math> (5000Hz)</p> <p>10<math>\mu\text{s}</math> (100kHz)</p>	<p>Probe moving at 2 mm/sec, therefore 5000 A pulses per second.</p>
 <p>10<math>\mu\text{s}</math> (100kHz)</p>	<p>Probe moving at 50 mm/sec, therefore limited to Maximum Output frequency (100 kHz)</p>

# Frequency of Pulses

---

## ATM system Lag

Once the probe is moving sufficiently fast that its Output Signal Frequency is limited by the factory set Maximum Output Signal Frequency then lag will be introduced into the measurement. This must be considered if the ATM is being used in a control application.

## ATM Bandwidth

The ATM has a measurement bandwidth of 100 Hz. If it is used to measure signals with a frequency greater than 100 Hz then information about this signal will be lost.

# Receiver Electronics

---

The receiver electronics must be able to handle signals up to 4 times the Maximum Output Signal frequency to ensure correct operation and not lose count.

ATM Maximum Output Signal Frequency	Minimum Frequency for Receiver
kHz	kHz
50	200
100	400
125	500
180	720
250	1000
360	1440
500	2000

Table 2: Receiver Electronics Input Frequency Requirements

# Pre and Post Travel Positions

The ATM is set so that the probe has a pre and post travel region outside of the measurement range. If the probe is within the pre or post travel no signals are transmitted.

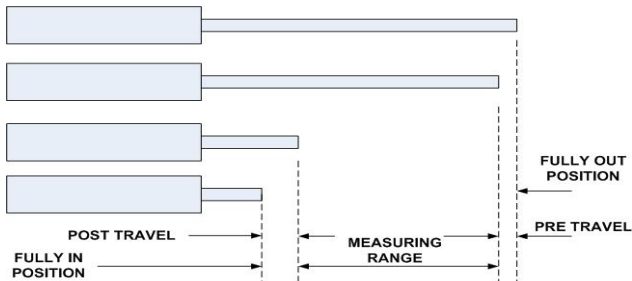


Figure 5: Pre and Post Travel

# Absolute Mode and Incremental Mode

---

These options can be factory set.

In Absolute mode, on power on the ATM will read its absolute position and send pulses to the receiver corresponding to this position.

In incremental mode, on power on the ATM will treat this position as zero and will not send any pulses until it is moved.



# Indication Lamps

---

The ATM has two indication lamps.

Condition	Blue LED	RED LED
Probe Moving (>10 $\mu$ m)	Flash	
Low Voltage warning (ATM still operates) **		Flash 20% On 80% Off
Low or High Voltage Error		Flash 80% On 20% Off
Hardware Error		On

\*\* The ATM requires a +5 V  $\pm$  0.25 VDC Supply. If the voltage is outside of this range a warning is indicated, however the ATM will continue to operate. If the voltage is worse than 0.5 V out of range an error is indicated and the ATM stops transmitting signals.

# Technical Data

---

<b>Measurement Performance</b>	
Transducer Range	0.5 mm to 150 mm depending on Probe Type fitted
Accuracy	Up to 0.15% reading depending on probe Type fitted
Resolution (x 4 interpolation)	0.1, 0.2 or 0.5 $\mu\text{m}$ (factory set)
Repeatability	<0.15 $\mu\text{m}$ depending on Probe Type Fitted
<b>Electrical Performance</b>	
Power	+5 V $\pm$ 0.25 VDC @ 100 mA
Output Signals (differential)	A and B, /A and /B (TTL / RS422)
Maximum Output Frequency	50, 100, 125, 180, 250, 360, 500 kHz (factory set)
Bandwidth	100 Hz

# Technical Data

---

<b>Environmental</b>	
Sealing	Transducer: typically IP65 depending on type. Electronics Module IP43
EMC	EN61000-6-3 Emissions EN61000-6-2 Susceptibility
Operating Temperature	0 °C to 60 °C
Storage Temperature	-20 °C to 70 °C
Air Supply (Pneumatic Probes)	Clean and Dry Air, maximum RH 60%, filtered to better than 5 µm (0.1 µm for specialist transducers with ultra low tip force). If unsure check with factory.
Operating Pressure (Pneumatic Probes)	Depends on Probe Type fitted. If unsure check with factory.

# Electrical Connections

---

The ATM is normally supplied with 2 m of cable between the probe and the electronics module and 1 m between the electronics module and the connector or free wire end.

Signal	Description	Wire Ended	15 Way D Type (Heidenhain Pin Out)	15 Way D Type High Density
A	In Phase	Red	1	1
/A	In Phase Inverted	Pink	9	2
B	Quadrature	Yellow	3	3
/B	Quadrature Inverted	Green	11	4
Supply (+5 V $\pm$ 0.25 VDC)	Power Supply	Blue	4 & 12	13
Return (0V)	Return (0V)	Black	2 & 10	14